FREEDOM DIAGNOSTICS

Proudly Owned and Operated in the USA

Searchable via: FreedomDiagnosticsTesting.com

# Certificate of Analysis

| | |
|---|---|
| **Accession Number** | 2602110116 |
| **Client** | Unique Chemx |
| **Search Code** | Uniq2602110116 |

| | |
|---|---|
| **Received Date:** | 02/11/2026 |
| **Reported Date:** | 2/12/2026 |

| | |
|---|---|
| **Product** | Ipamorelin 10mg |
| **Net Peptide Content** | 10.42 mg |
| **Identity** | Ipamorelin |

| | |
|---|---|
| **Lot** | IP10-260112-01 |
| **Purity** | 99.856% |
| **Appearance** | White Lyophilized Powder |

**All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry**

| Mass Identification | Result |
|---|---|
| **Ipamorelin** | **99.856%** |

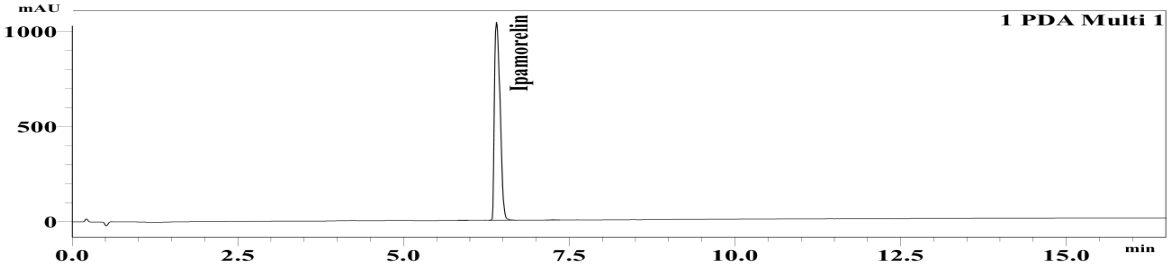

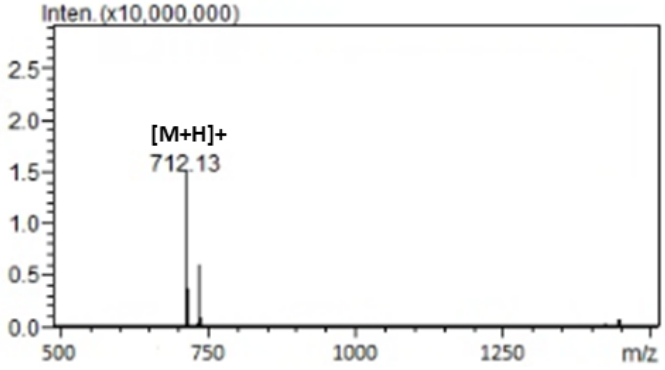


*Stephen Schmidt*

Stephen Schmidt

Principal Chemist

## COA: 2602110116

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

# Certificate of Analysis

FREEDOM DIAGNOSTICS

Proudly Owned and Operated in the USA

Searchable via: FreedomDiagnosticsTesting.com

| | |
|---|---|
| **Accession Number** | 2602110117 |
| **Client** | Unique Chemx |
| **Search Code** | Uniq2602110117 |

| | |
|---|---|
| **Received Date:** | 02/11/2026 |
| **Reported Date:** | 2/12/2026 |

| | |
|---|---|
| **Product** | Ipamorelin 10mg |

| | |
|---|---|
| **Lot** | IP10-260112-01 |

**All analyses are conducted for research purposes and performed in duplicate in accordance with USP <85> guidelines. *Endotoxin limits are established per USP <85> Bacterial Endotoxins Test and USP <161> Medical Devices—Bacterial Endotoxin and Pyrogen Tests.**

| Endotoxin Threshold | Result |
|---|---|
| **Replicate 1** | **Pass** |
| **Replicate 2** | **Pass** |

Stephen Schmidt

Stephen Schmidt
Principal Chemist

## COA: 2602110117

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.